
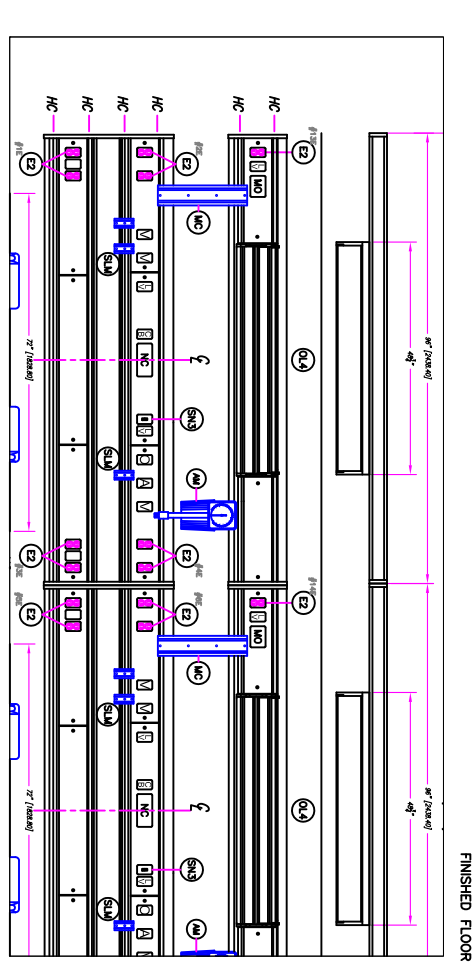


# MAJESTIC SERIES HORIZONTAL HEADWALL SYSTEM

THREE TIER WITH NO CHASE  
(M/N: HW00-03T-S-M288)

DRAWING # 42

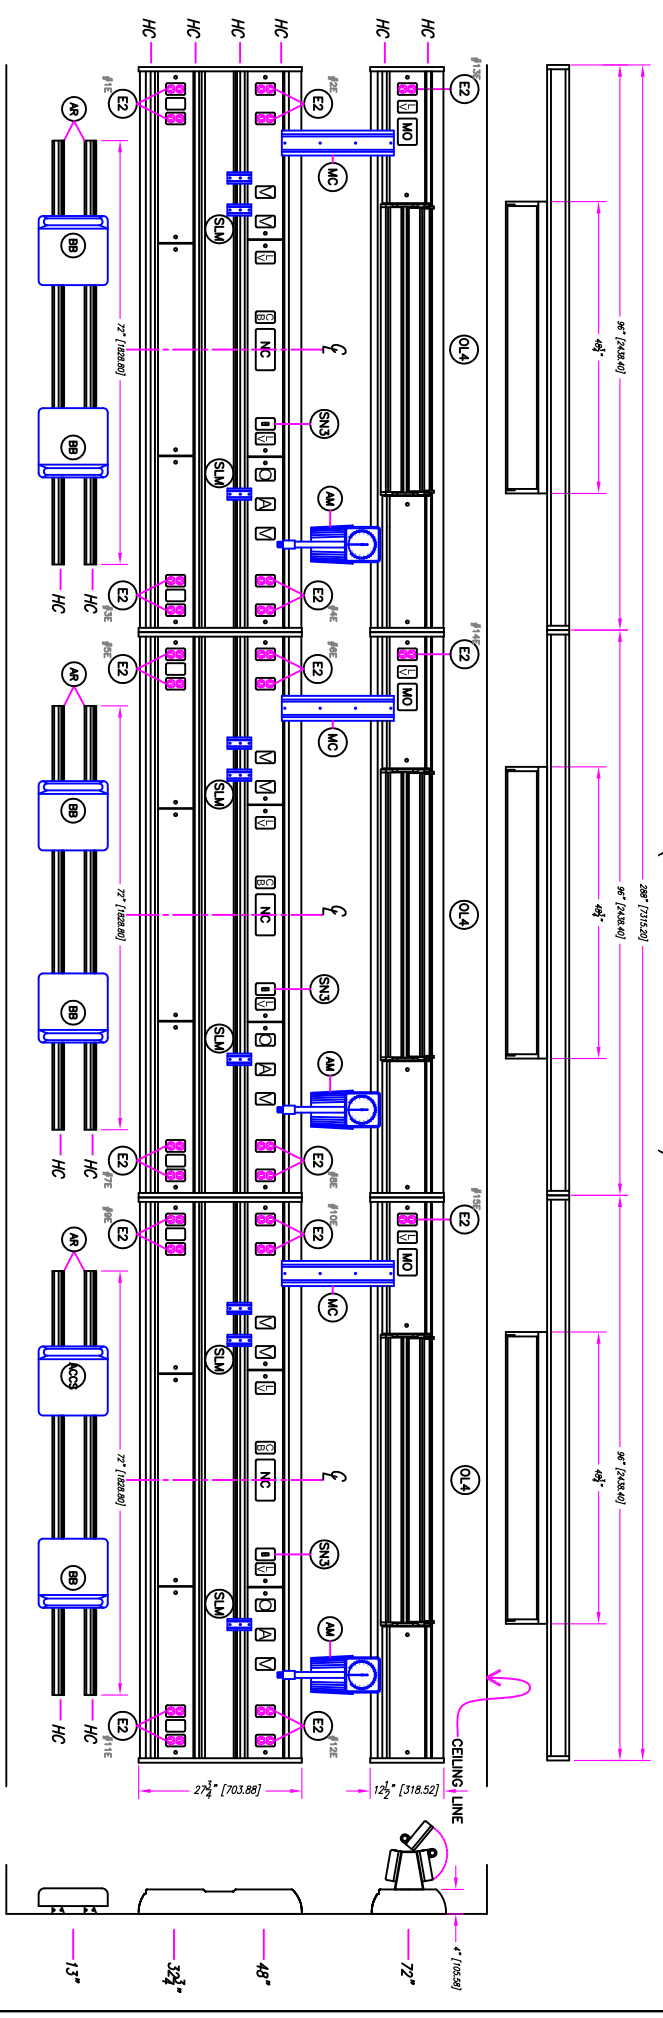

TYPE:  
QUANTITY:

SYMBOL	QTY.	DESCRIPTION
HC	6	HORIZONTAL EQUIP. TRACK
O	3	GAS, OXYGEN
A	3	GAS, MED AIR
V	9	GAS, VACUUM
E2	27	RECEPTACLE - DUPLEX RED
SN3	3	SWITCH, 3 POSITION L.V.
NC	3	PROVISION - NURSE CALL 3G
CB	3	PROVISION - CODE BLUE 1G
LV	9	PROVISION - LOW VOLTAGE 1G
M/O	3	PROVISION - MONITOR OUT 2G


SLM	9	VACUUM SLIDE, TRACK MTD.
OL4	3	4" OVERBED LIGHT
LVC*	3	LOW VOLTAGE CONTROLLER
MC	3	MONITOR CHANNEL, TRACK MTD.
AM	3	ANEROID MANOMETER w/ BSKT
AR	6	AMICO RAIL SYSTEM, WALL MTD.
BB	3	BED BUMPERS, TRACK MTD.

\*INSTALLED IN OVERBED LIGHT BY AMICO

IMPORTANT: PLEASE VERIFY THAT THE ABOVE INFORMATION IS CORRECT, AND PROVIDE THE REMAINING DETAILS.

APPROVAL - PRINT AND SIGNATURE \_\_\_\_\_

DATE \_\_\_\_\_ PHONE NO. \_\_\_\_\_



**AMICO** Corporation  
85 Fulton Hwy,  
Rehoboth Hill, Ontario  
L4B 2N4, CANADA  
Tel: (905) 877-462-6426(F)  
Toll-Free: 1-877-462-6426(F)  
Fax: (905) 764-0860  
www.amico.com

HOSPITAL LOCATION \_\_\_\_\_ HOSPITAL LOCATION \_\_\_\_\_

QTY. 1 ( ) TYPE \_\_\_\_\_ UNITS AS SHOWN / ( ) TYPE \_\_\_\_\_ UNITS OPPOSITE \_\_\_\_\_

A. NURSE CALL MFR: \_\_\_\_\_ MODEL NO.: \_\_\_\_\_

B. MEDICAL GAS MFR: \_\_\_\_\_ TYPE CONNECTION: \_\_\_\_\_

C. FINISH: \_\_\_\_\_ CEILING HEIGHT: \_\_\_\_\_

DRWG. NO. PRJ03900K-46  
DRAWN BY: \_\_\_\_\_  
CHECKED BY: \_\_\_\_\_  
REV. NO.: \_\_\_\_\_  
DATE: \_\_\_\_\_