Accessories AMICO

Instruction Manual

VRS RAIL INSTALLATION

the right **connection**

www.amico.com

Amico Accessories Vertical Rails are designed to help make device mounting easier. Vertical Rails are superior equipment management systems used to improve the ergonomics of health care facilities.

(VRS) VERTICAL RAIL SYSTEMS:

• Mount flush to any surface

• Designed for vertical applications

• Can be used in conjunction with horizontal rails

• Ideal for inlaying in cabinets/case work

• Laminate inserts and end caps can be added

• Available in a wide variety of lengths

MOUNTING REQUIREMENTS

Vertical Rail, #12 x 2½" High Tensile Phillips Sheet Metal or Wood Screws ***NOTE:** Amount of screws varies depending on channel length.

MEDICAL FACILITY RESPONSIBILITY

Amico Vertical Rails must be inspected periodically. Assure the proper backing in the wall is installed prior to adding rails. A defective product should not be used. Parts that are broken, missing, plainly worn, distorted or contaminated, should be replaced immediately. Should such repairs or replacements become necessary, please contact your local distributor.

ALTHOUGH CONSIDERABLE EFFORT HAS BEEN MADE TO ENSURE THE SAFETY IN THIS MANUAL THE INSTALLATION ITSELF IS BEYOND THE CONTROL OF AMICO ACCESSORIES INC. ACCORDINGLY, AMICO ACCESSORIES WILL NOT BE RESPONSIBLE FOR THE FAILURE OF ANY SUCH INSTALLATION.

***WARNING:** IT SHALL BE THE RESPONSIBILITY OF THE HOSPITAL, ITS CONSULTANTS AND/OR CONTRACTORS TO DETERMINE THAT THE WALL IS ADEQUATE TO SAFELY MOUNT THE SPECIFIC INSTRUMENT. THIS INCLUDES THE SELECTION OF APPROPRIATE FASTENERS AND THE PROPER INSTALLATION. THE FOLLOWING IS GUIDELINE INFORMATION ONLY. SEE RAIL INSTRUCTIONS FOR SPECIFIC WALL CHANNEL GUIDELINE INFORMATION.

***WARNING:** A LATERAL FORCE OF 80LBS APPLIED 17" OUT FROM THE WALL WILL CRACK A 5/8" THICK GYPSUM BOARD ALONG THE CHANNEL FLANGE.

THIS IS NOT ACCEPTABLE IN SEISMIC SENSITIVE AREAS AND IN CALIFORNIA.
FOR MORE INFORMATION ON CALIFORNIA'S SEISMIC LAWS PLEASE VISIT HTTP://WWW.CA.GOV

CHANNEL PLACEMENT

1. Place the bottom end of the rail 56" above the floor.
***NOTE:** Some devices may require lower rail placement.

2. The bottom of the device should be 4½" above the bottom of the rail. Access to device controls should be considered before mounting the rail.

3. Allow 14" clearance on either side of the rails center line to clear objects such as over-bed lighting, privacy curtains, adjacent walls or columns, door swing arcs, etc. Power and signal outlets should be considered when selecting a rail location. Avoid oxygen, vacuum outlets and attendant flow meters, and don't place any portion of the device over a patients bed.

DRYWALL OVER STEEL OR WOOD STUDS

1. Locate studs and mark the desired area where your rail will be mounted.

2. Drill 11/64" (17mm) diameter holes into the rail 2" from the top and bottom of the rail for the



VERTICAL RAIL

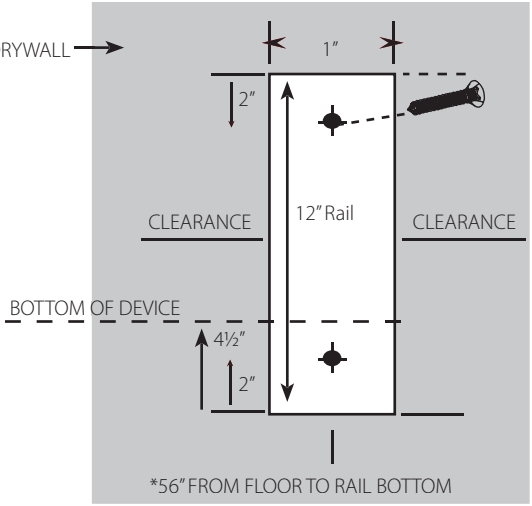

WARRANTY

During the term of your warranty: Within the first twelve (12) months from the date of shipment Amico Accessories will repair or replace any part which is proven to be defective at our cost. After the twelve (12) months Amico Accessories will send the parts to the customer free of charge, but the shipping and installation will be borne by the customer.

The warranty is valid only when the product has been properly installed according to Amico Accessories specifications used in a normal manner and serviced according to factory recommendations. It does not cover failures due to damage which occur in shipments or failures which resulted from accidents, misuse, abuse, neglect, mishandling, alteration, misapplication or damage that may be attributable to acts of God.

AMICO ACCESSORIES DOES NOT HONOR VERBAL STATEMENTS CONCERNING THE WARRANTY.

The distributor and/or dealer are not sanctioned to create verbal warranties about the product described in this agreement. Any statements will not be honored or be made part of the agreement of sale. This document is the final complete and exclusive terms of the agreement.

THIS WARRANTY IS INCLUSIVE AND REPLACES ALL OTHER WARRANTIES.

Amico Accessories shall not, under any circumstances be liable for incidental or consequential damages including, but not limited to, profit, loss of sales or injuries to person(s) or property. Correction of non-compliance as noted above will result in completion of all liabilities of Amico Accessories whether based on agreement, neglect or changed materials, designs or specifications without notice.

All claims for warranty must first be approved by Amico Accessories Service Department: (info@amico-accessories.com or 1.877.AMICO XS). A valid Return Goods Authorization number must be obtained from Amico Accessories prior to commencement of any warranty claim.

Amico Accessories Inc.
85 Fulton Way, Richmond Hill
Ontario, L4B 2N4

Toll Free Tel: 1–877–264–2697
Tel: 905–763–7778
Fax: 905–763–8587
E-mail: info@amico-accessories.com

Please visit www.amico.com for more information on our product installation instructions.

IM-VRS079
Printed June 07